



ASIAN HARMONIZATION
WORKING PARTY



INDONESIA

UPDATED
MEDICAL DEVICE REGULATION

Presented by
ARIANTI ANAYA
Director of Medical Device Production and
Distribution Service

MINISTRY OF HEALTH REPUBLIC OF INDONESIA



Presented at
17th AHWP Meeting
TICC – Taipei,
5 November 2012



UPDATES OUTLINE



Background

Medical Device
Regulation in Indonesia


National Medical Devices Policy

Indonesia Regulation System for
Medical Devices

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



INDONESIA: Gateway to ASEAN

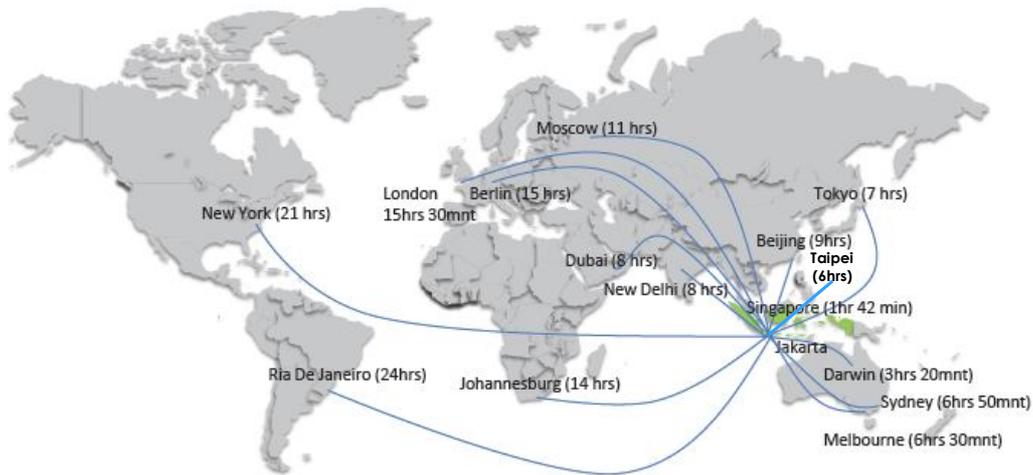

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia

UNIVERSAL COVERAGE



- ◆ Medicines
- ◆ Medical Devices



UNIVERSAL
COVERAGE
1 Jan 2014

- Important component in the healthcare system
- Tight related with technology and economy
- One of trade commodity and social need





INDONESIA MEDICAL DEVICE OVERVIEW



- Population > 240.000.000
- Human Dev. Index = 0.6 (medium)
- GDP per capita = \$ 3.015
- Medical Devices Manufactures = 234
- Medical Devices Suppliers > 800
- Registered Medical Devices (2011)
 - Import = 37.851 items
 - Local = 3.872 items
- Market values for medical device (2011) : USD 780 m

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia




LEGAL BASIS REGULATION




1. Act on health
2. Gov. Regulation: Law enforcement
3. MoH: Production
4. MoH: Distribution
5. MoH: Registration of Medical Devices and House Hold Production



ORGANIZATIONAL STRUCTURE

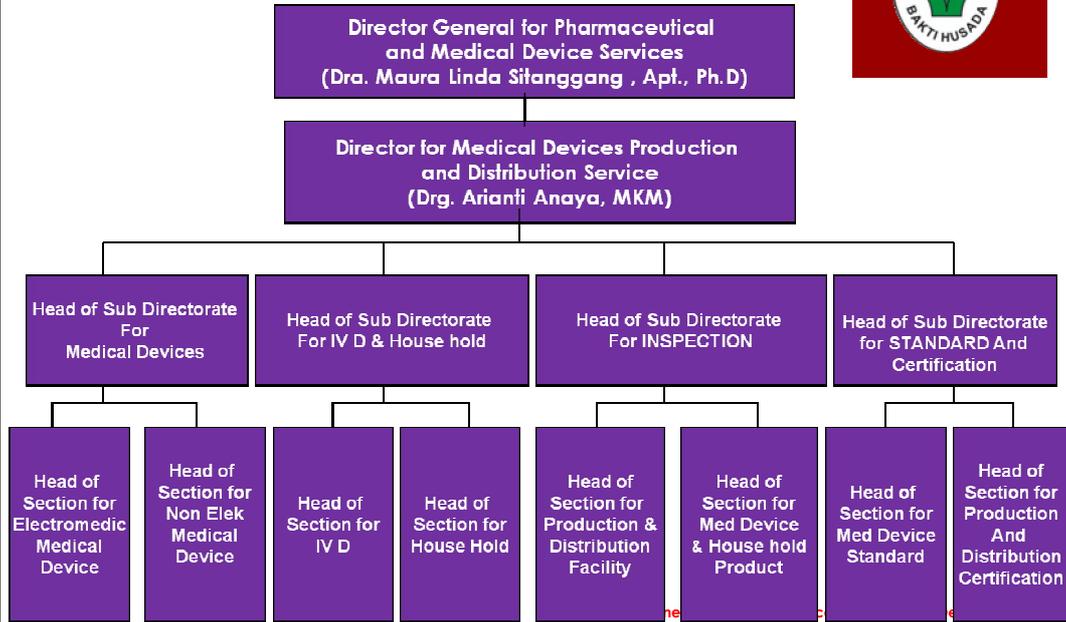

NATIONAL MEDICAL DEVICE POLICY

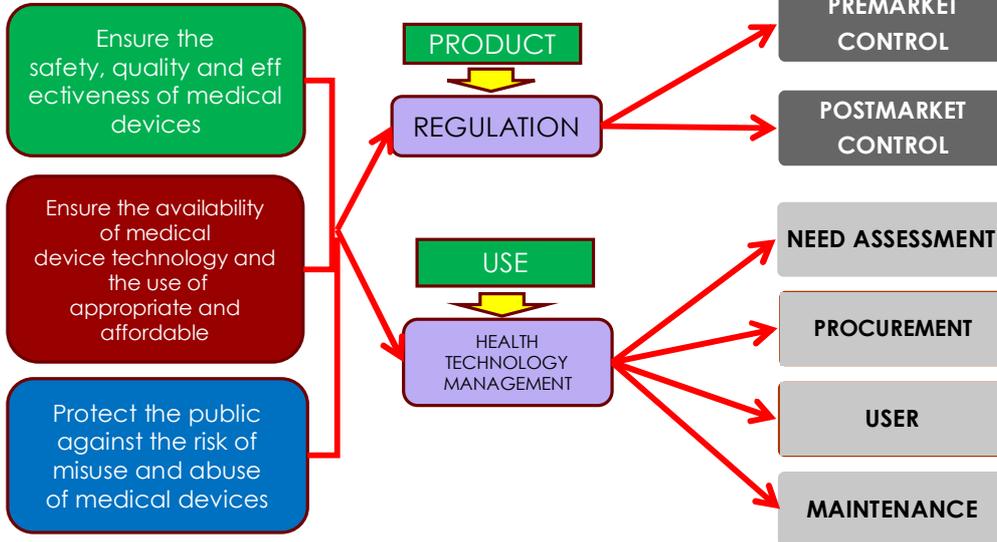

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



GOALS OF THE REGULATORY SYSTEM IN INDONESIA



Risk Based Approach

- Both product risk and compliance risk can be managed by premarket activities and post market activities

ASEAN HARMONIZATION

- Indonesia which one of ASEAN members economies will have the same vision to achieve the ASEAN Economy Society

International Standard

- Indonesia as one of world Nation, has the same standard of quality that use in global harmonization regulation

Transparency and excellent service

- One of the priority of Indonesian Health reformation is strengthen the public service

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



PREMARKET CONTROL



- For registration requirement, Indonesia has adopted:
 1. Common Submission Dossier Template CSDT
 2. ISO 13485 for Quality Management System
 3. National and International Standard for ensuring the safety, quality and effectiveness of medical device
- Validity of registration number: 5 years
- All classification of medical device must get registration number before entering the Indonesia territory.
- Spare part and accessories, is not required to be registered
- All accessories of the product will attached in registration number in order to simplify the custom release

Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



Example for Registration License



MINISTRY OF HEALTH OF THE REPUBLIC OF INDONESIA
DIRECTORATE GENERAL OF PHARMACEUTICAL AND MEDICAL DEVICES DEVELOPMENT
 J. H. R. Rasuna Said Blok X5 Kavling No. 4-9 Jakarta 12950
 Phone: +6221-6201890 (Hunting) Facsimile: +6221-62964838 Po BOX 203

In accordance with:
 The Regulation of The Minister Health Of The Republic Of Indonesia No. 1190/Menkes/Per/VIII/2010 dated August 23, 2010 regarding Medical Devices and Household Products Registration License

Herby given the marketing licence under:

NUMBER OF REGISTRATION LICENSE
MEDICAL DEVICE
 KEMENKES RI AKL.20502214455

Name of Product : **ROHTO Neo Eye Foldable Lens**
 Generic Name : Intraocular Lens
 HS Code : 9022.14.00.00
 Category : Eye Device
 Sub Category : Prosthetic Eye Device
 Type/Size : RF-22L/ Dioptre +4 s/d +40
 Packaging : Box Containing Lens Holder @ 1 Lens
 Name of Manufacturer : PT. ROHTO LABORATORIES INDONESIA, PADALARANG
 Name of Distributor : PT. ROHTO LABORATORIES INDONESIA, PADALARANG
 Under License from : -
 Stipulation : 1. This registration license is valid within
 2. Submit the periodical report every 1 (one) year concerning type and side effect of the marketing products is an obligation

Rules and Regulations : 1. if on the other day there is another party who has a right upon the above agency appropriate with the valid regulation, the agency should be willing to release of the distributor authorization for the product.
 2. if on the other day there is any fault, this license will be reviewed.

Jakarta,, 20...
 On behalf of Director General,
 Director for
 Medical Device Production and Distribution Development,

Dra. Nasrah Bahaudin, Apt., MM
 NIP. 19631031 198601 2 001

Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia

Obviously described



Example for Attachment Accessories or Type Registration License



MINISTRY OF HEALTH OF THE REPUBLIC OF INDONESIA
DIRECTORATE GENERAL OF PHARMACEUTICAL AND MEDICAL DEVICES DEVELOPMENT
 Jl. H. R. Rasuna Said Blok X5 Kavling No. 4-9 Jakarta 12950
 Phone: +621-5201590 (Hunting) Facsimile: +621-52964338 PO BOX 203

Attachment

**NUMBER OF REGISTRATION LICENSE
 MEDICAL DEVICE
 KEMENKES RI AKL 2009214455
 Dated February 21, 2012**

NO	TYPE	SIZE	PACKAGING BOX
1	RE-01	Diopter + 4 s/d + 40	1 piece
2	RE-02	Diopter + 4 s/d + 40	1 piece
3	RE-03PH	Diopter + 4 s/d + 40	1 piece
4	RE-04PH	Diopter + 4 s/d + 40	1 piece
5	RE-05	Diopter + 4 s/d + 40	1 piece
6	RE-06	Diopter + 4 s/d + 40	1 piece
7	RE-06F	Diopter + 4 s/d + 40	1 piece
8	RP-11	Diopter + 4 s/d + 40	1 piece
9	RP-12	Diopter + 4 s/d + 40	1 piece
10	RP-13	Diopter + 4 s/d + 40	1 piece
11	RJ-51	Diopter + 4 s/d + 40	1 piece
12	RJ-51PH	Diopter + 4 s/d + 40	1 piece
13	RA-15	Diopter + 4 s/d + 40	1 piece
14	RA-25	Diopter + 4 s/d + 40	1 piece
15	RA-25	Diopter + 4 s/d + 40	1 piece

Number of Registration License of Medical Device only valid for Type, Size, and Packaging are listed in this attachment.

Jakarta, 20

On behalf of Director General,
 Director for
 Medical Device Production and Distribution Development.

Dra. Nasrah Bahaudin, Apt., MM
 NIP. 19531031 198501 2 001

al and Medical Device Service
 of Health of Republic Indonesia

Obviously described



Obviously described



Indonesia national single window

- National Single Window (NSW) is a national system that will integrate all entities which related to customs release and clearance of cargoes with the aim of accelerating the settlement process of import-export services and increased effectiveness and performance of traffic handling import-export goods.



Indonesia Trade Repository

- repository contains trade rules and regulations through the existing Indonesian National Single Window (INSW) portal. The information in INTR are about HS code, regulation issued by Government Authority's related to import or export permit license , exchange rates, rules of origin and also trade simulation.

www.eservice.insw.go.id

Single Sign On

- Is a facility to provide users with single and simultaneous access to INSW and licensing systems.
- Once logged in to the system, users do not have to log in to other INSW-affiliated systems (once signed-in, multiple access)



Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



e-REGISTRATION FOR MEDICAL DEVICE



<http://regalkes.depkes.go.id>

BACKGROUND



- Wide area of Indonesia territory
- Optimize public service
- Quick registration system and can be access anywhere



Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia



FEATURES In e-REGISTRATION



Directorate General of Pharmaceutical and Medical Device Service
Ministry of Health of Republic Indonesia

DISTRIBUTION



Who can distribute Medical Device in Indonesia ?



Company which have Distribution license issued by MOH



DISTRIBUTOR
• Good Distribution Practice



A routine assessment for all Distributors by MOH



POST MARKET CONTROL

SAMPLING

- A routine activity to taking sample from market and then testing it to laboratory for compliance check

MONITORING

- A routine activity to audit the production and distribution facilities compliance with Quality System standard

VIGILLANCE

- A program activity for Adverse event report



Post Market Surveillance

PMS should supported by strict law enforcement



To control the PMS, MOH have government Civil police Investigator for medical devices who works together with Hospital/Healthcare facilities, police, custom and Health province officer



THANK YOU / 谢谢

